




Engineered For Your Mission

Gazelle Series Rescue Litters
USER MANUAL
 PROFESSIONAL USE

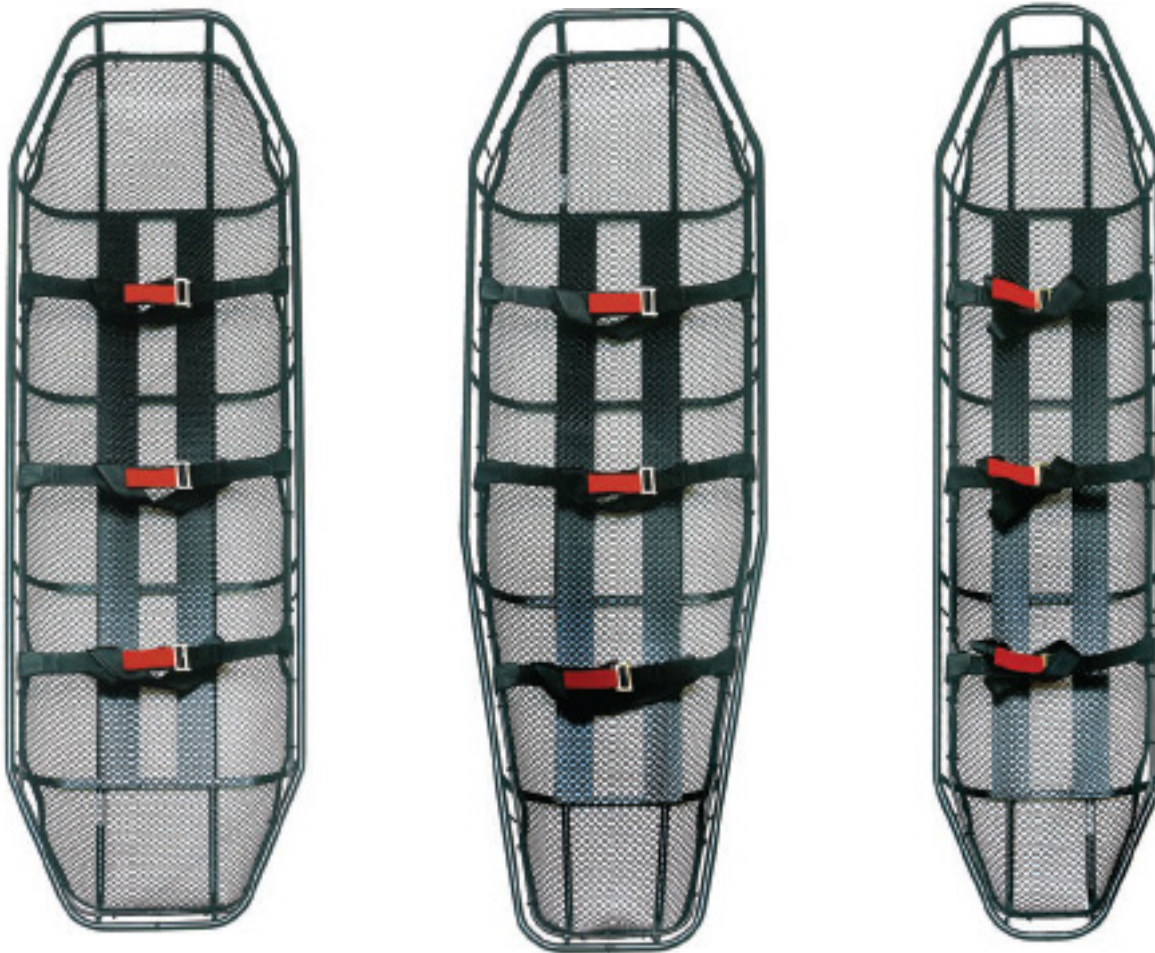

Model 11-0105Gazelle Rescue Litter, Regular

Model 11-0106Gazelle Rescue Litter, Tapered

Model 11-0107Gazelle Rescue Litter, Confined Space

Model 11-0105BGazelle Rescue Litter, Regular (Black)

Model 11-0106BGazelle Rescue Litter, Tapered (Black)

Model 11-0107BGazelle Rescue Litter, Confined Space (Black)



Read this Manual and Retain
 for Future Reference

TABLE OF CONTENTS / GAZELLE SERIES RESCUE LITTERS

Disclaimer 3
 Adverse Event Notice..... 3
 Proprietary Notice..... 3

1. Safety Information 3
 1.1 Warnings..... 3
 1.2 Important..... 3
 1.3 Bloodborne Disease Notice 3
 1.4 Safety Labels 4

2. Operator Skills and Training 4
 2.1 Skills..... 4
 2.2 Training 4

3. About the Rescue Litter..... 4
 3.1 General Specifications 4

4. Restraints 4
 4.1 About the Restraints 4
 4.2 Fastening and Tightening the Restraints..... 4
 4.3 Loosening and unfastening the Restraints 5
 4.4 Attaching the Restraints 5

5. Using the Rescue Litter 5
 5.1 Before Placing the Rescue Litter in Service..... 5
 5.2 General Guidelines for Use 5
 5.3 Carrying the Rescue Litter..... 5
 5.4 Sliding the Rescue Litter 5

6. Maintaining the Rescue Litter 6
 6.1 Maintenance Schedule..... 6
 6.2 Disinfecting and Cleaning the Restraints 6
 6.3 Disinfecting and Cleaning the Rescue Litter 6
 6.4 Inspecting the Rescue Litter..... 6
 6.5 Storing the Rescue Litter 6

7. Repair, Parts and Service..... 6
 Accessories 6
 Related Products..... 6

8. Limited Warranty 7

9. Traverse Customer Care 7
Training Schedule..... 8
Maintenance Record..... 8

Disclaimer

This manual contains general instructions for the use, operation and care of this product. The instructions are not all-inclusive. Safe and proper use of this product is solely at the discretion of the user. Safety information is included as a service to the user. All other measures taken by the user should be within and under consideration of applicable regulations. It is recommended that training on the proper use of this product be provided before using this product in an actual situation.

Retain this manual for future reference. Include it with the product in the event of transfer to new users. Additional free copies are available upon request from Customer Care.

Refer to this manual before and after each use. Failure to follow instructions for use and maintenance may result in serious consequences for the operator and/or patient.

Adverse Event Notice

In the event of an adverse event or serious incident related to the use of this device, the end user/operator must report the incident to Traverse Rescue LLC at 2715 Bristol Circle, #2, Oakville, Ontario L6H 6X5, (905) 279-7866, or via email at info@traverserescue.com. If the incident occurred in the European Union, report it to Traverse's Authorized EU Representative and the competent authority of the Member State in which the end user is established.

Proprietary Notice

The information disclosed in this manual is the property of Traverse Rescue, LLC., Oakville, ON Canada. Traverse Rescue, LLC. reserves all patent rights, proprietary design rights, manufacturing rights, reproduction use rights, and sales use rights thereto, and to any article disclosed therein except to the extent those rights are expressly granted to others or where not applicable to vendor proprietary parts.

© Copyright Traverse Rescue, LLC. All Rights Reserved

Traverse Rescue, LLC.
2715 Bristol Circle, Unit 2
Oakville, Ontario
Canada L6H 6X5

Telephone:905 279 7866
Toll Free (Canada & US):1 866 998 7866
Fax :905 615-1199
www.traverserescue.com

EC	REP	Ferno s.r.l. Via B.Zallone, 26 40066 Pieve di Cento, Italy +39 0516860028
----	-----	--



UK	REP	Ferno (UK) Limited Stubs Beck Lane, Cleakheaton West Yorkshire BD19 4TZ, United Kingdom 44 (0) 1274 851999
----	-----	---



Traverse Rescue, LLC manufactures its products under a strict Quality Management Program. We also recognize and comply to any applicable standards that apply to each product.

Rescue Litters manufactured by Traverse Rescue, LLC have been determined to be Class 1 Medical Devices.

1. Safety Information

1.1 Warnings

The following are warnings in this manual:

WARNING
Untrained operators can cause injury or be injured. Permit only trained personnel to operate this Rescue Litter.
Improper use of the Rescue Litter can cause injury. Use the Rescue Litter only for the purpose described in this manual
An unrestrained or improperly restrained patient can suffer injuries. Always secure the patient in the Rescue Litter with a restraint system suitable to the situation
Improper operation can cause injury. Operate the Rescue Litter only as described in this manual
An un-attended patient can be injured. Stay with the patient at all times
Helpers can cause injury or be injured. Maintain control of the Rescue Litter and direct all helpers
Improper maintenance can cause injury and damage. Maintain Rescue Litter only as described in this manual
Improper parts and service can cause injury. Use only Traverse-approved parts and service on the Rescue Litter
Modifying the Rescue Litter can cause injury and damage. Use the Rescue Litter only as-sold by Traverse.
Attaching improper or inappropriate items to the Rescue Litter can cause injury. Use only Traverse-Approved items on the Rescue Litter

1.2 Important

Boxes like the one below emphasize important information.

IMPORTANT
Traverse Gazelle series are for use within basic rescue and first response use and is not intended to be deployed within technical rescue scenarios such as: high angle rescue, over the edge rescue, helicopter hoist or short haul rescues. End users who choose to use the Traverse Gazelle Series of Litters in technical rescue scenarios, do so under their own responsibility and liability.

1.3 Bloodborne Disease Notice

OSHA (Occupational Safety and Health Administration) requires employers to protect workers from workplace exposure to bloodborne diseases such as HIV-1 and hepatitis. To reduce the risk of exposure when using the Rescue Litter, follow disinfecting and cleaning instructions in this manual.

1.4 Safety Labels

Labels place important information from the Users' Manual on the Rescue Litters.

Read and follow label instructions. Replace worn or damaged labels immediately. New labels are available from Traverse.

The Load-Limit label shown is affixed to the Rescue Litter.



2. Operator Skills and Training

2.1 Skills

Operators using the Rescue Litter need:

- A working knowledge of emergency patient-handling procedures.
- The ability to assist the patient
- A complete understanding of the procedures described in this manual

2.2 Training

Trainees need to:

- Follow a training program designed or approved by their training officer
- Read this manual. For additional free users' manual, contact Traverse Customer Care.
- Practice with the Rescue Litter before using it in regular service
- Be tested on their understanding of the Rescue Litter
- Record their training information

3. About the Rescue Litter

3.1 General Specifications

Polyethylene Netting...-65°F/-54°C to +200°F/+93°C

Restraint Webbing

Tensile Strength.....975 lbs. / 442 kg

Load Rating500 lbs. / 227 kg

Restraint Buckles

Minimum Tensile Load.....4000 lbs. / 1814 kg

Buckles meet ANSI Z359.1 and CSA Z259.1

Traverse Rescue LLC reserves the right to change specifications with out notice.

Gazelle Series Rescue Litter			
Length (Regular & Tapered)	82.5 in	209.6 cm	2096 mm
Width (Regular & Tapered)	24.5 in	62 cm	620 mm
Depth (Regular & Tapered)	7 in	18 cm	180 mm
Weight (Regular & Tapered)	33 lbs	15 kg	
Length (confined space)	82.5 in	209.6 cm	2096 mm
Width (confined space)	18.25 in	46.4 cm	464 mm
Depth (confined space)	7 in	18 cm	180 mm
Weight (confined space)	31 lbs	14 kg	
Rated Load Limit	900 lbs	4 kN	

WARNING

Untrained operators can cause injury or be injured. Permit only trained personnel to operate the Rescue Litter.

IMPORTANT

Rescue procedures using ropes, harnesses, bridles and other Personal Protective Equipment require special skills and are potentially hazardous activities. No rescue personnel should attempt such rescue procedures unless he or she has received professional instruction and training.

4. Restraints

4.1 About the Restraints

A total of four restraints are included with this Rescue Litter.

These restraints are to supplement what you will typically use to tie-in a patient. We have made them to a suitable strength in order to complement your own system of tubular webbing, cord or the like. These restraints are only for securing the patient into the Rescue Litter, and are not to be used for lifting or for any other purpose. Restraints are considered a consumable item and can be replaced. (section #7)

4.2 Fastening and Tightening the Restraints

The strap with the three-bar buckle is constructed with a looped end that attaches to the Rescue Litter, and a free end that is used to tighten the restraint (figure 1).

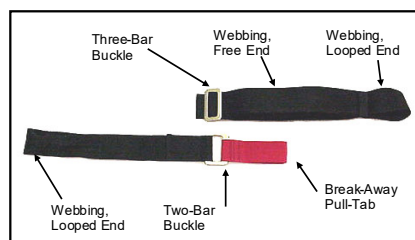


Figure 1, Components

1. Pass the three-bar buckle and webbing upward through the opening in the two-bar buckle (fig. 2). Make sure to pull the free end of the webbing completely through the opening.

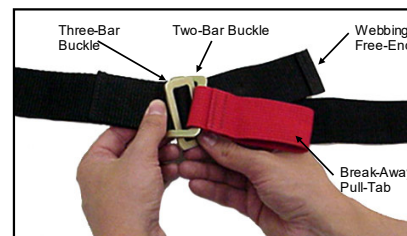


Figure 2, Fastening the Buckle

2. Pull slightly on the free end of the webbing to firmly seat the three-bar buckle on top of the two-bar buckle (fig. 3).

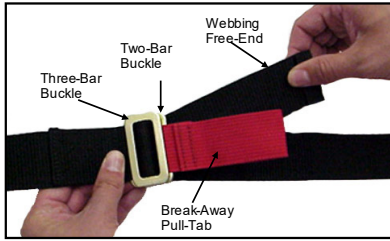


Figure 3, Seating the Buckles

3. Tighten the restraint by pulling on the free end of the webbing.

4.3 Loosening and unfastening the Restraints

To loosen a restraint, pull the breakaway tab toward the buckle (fig. 4). Continue pulling until the restraint is as loose as desired.



Figure 4, Loosening Restraint

To unfasten the restraint, first loosen as in step number 1, then angle the three-bar buckle and pass it downward through the opening in the two-bar buckle (fig. 5).

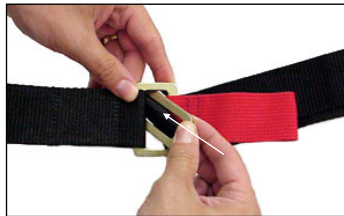


Figure 5, Unfastening Buckle

4.4 Attaching the Restraints

The top edge of the High Density Polyethylene netting is shaped with coves to provide points where restraints can easily be fastened to the lower-rail of the Rescue Litter (fig. 6).



Figure 6, Restraint Cove

Select attachment points that are appropriate for effective securing of the patient, as well as for working together with your own fastening system.

Attach the supplied restraint as follows:

1. Unfasten the buckle to separate the restraint straps.
2. Starting outside the Rescue Litter, pass the looped end of the strap inward between the Rescue Litter rail and the netting at a chosen attachment point. (Fig. 7)



Figure 7, Passing Looped End Through Cove

3. Thread the buckle through the restraint loop (Fig. 8) and pull until the loop is tight around the Rescue Litter rail.




Figure 8, Threading Buckle

4. Attach the remaining strap to the opposite side of the Rescue Litter following steps 2 and 3.

5. Using the Rescue Litter

5.1 Before Placing the Rescue Litter in Service

- Personnel who use this Rescue Litter are required to read this manual.
- If using the supplied restraints, attach them as instructed in **4.4 Attaching the Restraints**.
- Confirm that the Rescue Litter, restraints and mesh netting are in good condition. Follow instructions in Inspecting the Rescue Litter in this manual.

5.2 General Guidelines for Use

- The Rescue Litter requires a minimum of two trained operators. In most situations, operators may require additional help. For information about placement and direction of helpers, see **5.3 Carrying the Rescue Litter** in this manual.
- Follow standard emergency patient-handling procedures when using the Rescue Litter.
- Stay with the patient at all times.
- Always use the patient restraints provided, as well as a supplementary restraining system as per your training and team protocols, and the situation.
- Personnel using the Rescue Litter are responsible for learning the proper techniques involved, and for selecting the equipment and procedures best suited to the rescue situation.

5.3 Carrying the Rescue Litter

Carrying the Rescue Litter requires a minimum of two operators. Additional personnel will be helpful or even needed in most situations. Use an even number of personnel and position them to keep the Rescue Litter as even as possible.

Using Additional Help

Operators should maintain control of the Rescue Litter and direct any helpers.

5.4 Sliding the Rescue Litter

Slide the Rescue Litter on its runners over smooth surfaces. Avoid rock, stumps, branches or other hazards that could penetrate the netting, or cause discomfort or injury to the patient.

⚠ WARNING

Improper operation can cause injury. Operate the Rescue Litter only as described in this manual.

⚠ WARNING

An unattended patient can be injured. Stay with the patient at all times.

⚠ WARNING

An unrestrained or improperly restrained patient can suffer injuries. Always secure the patient in the Rescue Litter with a restraint system suitable to the rescue operation.

6. Maintaining the Rescue Litter

6.1 Maintenance Schedule

The Rescue Litter requires regular maintenance. Set up and follow a maintenance schedule, such as provided by the form below. This form represents minimum maintenance, and you can modify your own program based on your needs.

	Each Use	As Needed	Each Month
Disinfecting (6.3)	•		
Cleaning (6.3)		•	
Inspecting (6.4)		•	•

When using maintenance products, follow the manufacturers' directions and read the manufacturers' material safety data sheets.

⚠ WARNING

Improper maintenance can cause injury. Maintain the Rescue Litter only as described in this manual.

6.2 Disinfecting and Cleaning the Restraints

1. Remove restraints from Rescue Litter.
2. Buckle restraints before cleaning. This helps prevent damage to buckles or washing machine.
3. Place buckled restraints inside a mesh bag (not supplied) and place in an industrial washing machine.
4. Launder restraints in warm water, using a disinfectant soap and gentle agitation. Do not use bleach.
5. Remove restraints from mesh bag and hang to dry. Do not put restraints into home or commercial dryer.
6. Attach clean, dry restraints to Rescue Litter as instructed in Section 4.

6.3 Disinfecting and Cleaning the Rescue Litter

Wipe or spray all surfaces of Rescue Litter and netting with disinfectant. Follow disinfectant manufacturers' directions. Traverse recommends inspecting the Rescue Litter for obvious damage as you disinfect it.

Hand clean the Rescue Litter and netting with a mild detergent in warm water. Rinse well, and dry with a towel.

IMPORTANT

Disinfectants and cleaners containing bleach, phenolics, or iodine can cause damage to the restraints and Rescue Litter. Disinfect and clean only with products that do not contain these chemicals..

6.4 Inspecting the Rescue Litter

Have your stations/services' maintenance personnel check the following:

- All components should be present
- Weld joints should be free of cracks or any other sign of breakage
- Rescue Litter frame (top and lower rails, runners, ribs) should be free of dents, cracks or unintentional bends
- Polyethylene netting should be free of breaks and tears, and should be securely fastened to the lower rail.
- Warning labels should be clear and legible for all users to see and read.
- Restraint webbing should be in good condition with no cuts or frays
- Restraint buckles should be free of visible damage, and should operate properly.

If inspection shows damage or excessive wear, remove the Rescue Litter from service until appropriate repairs are completed (see Repair, Parts and Service, Section 7).

6.5 Storing the Rescue Litter

Store the Rescue Litter in a dry area. Make sure the Rescue Litter is clean and dry before placing it into storage.

7. Repair, Parts and Service

If your Rescue Litter is showing excessive wear or cracks (either in the material or at welds), it is time to retire it from service. Do not attempt to repair or replace any metal component or weld.

If the Mesh Liner, Patient Restraint straps or any labels are damaged and need repair, please call your Dealer or us to have them replaced.

Accessories

Always follow the instructions packaged with accessories. Keep the instructions with this manual. Be aware of any special considerations (loading heights, door heights, etc.)

Part Number	Description
05-0144	Traverse Rescue, Rescue Litter Cover
04-0108TR4	Traverse Restraint Strap - 4pk
05-0121	Rep. Mesh Gazelle (Regular)
05-0122	Rep. Mesh Gazelle (Tapered)
05-0123	Rep. Mesh Gazelle (Confined Space)

Related Products

Part Number	Description
11-0124A	2 Piece Floatation Collar
15-0240	Rescue Litter Handle
11-2220	Mule II Litter Wheel with handles

8. Limited Warranty

Traverse Rescue, LLC (Traverse) Limited Warranty states that all Traverse products are warranted for a period of one year after the date of invoice, to the original purchaser. This warranty is provided against any material or workmanship flaws or defects. In the event of such a flaw or defect during this warranty period, please contact Traverse Rescue immediately. Traverse Rescue, LLC agrees to repair or replace (at our choice) the defective product. Our Limited Warranty does not cover damage due to abuse, misuse, lack of care, improper use or accidents. It also does not cover damage due to attempted repair by the purchaser that was not authorized by Traverse Rescue, LLC. No other warranties exist or are implied by Traverse Rescue, LLC. This limited warranty excludes, and Traverse shall not be held liable for any punitive, incidental, special or exemplary damages arising out of the breach of the warranty on sales by Traverse or otherwise, or through the performance or non-performance of any third-party part, product, service or system. This limited warranty does not limit in any way, nor alter in any way, other manufacturer's warranties on products that are sold by Traverse Rescue, LLC.

9. Traverse Customer Care

Customer Care and product support are important aspects of each Traverse product.

For assistance with this, or any other Traverse product, please contact Traverse Customer Care.

Please have the serial number of your Traverse Rescue Litter available when calling Traverse Customer Care, and include this number with any written communications.

Traverse Rescue, LLC.
2715 Bristol Circle, Unit 2
Oakville, Ontario
Canada L6H 6X5

Telephone905 279 7866
Toll Free (Canada & US)1 866 998 7866
Fax905 615 1199
Emailinfo@traverserescue.com
Websitewww.traverserescue.com



